

Fig. 1

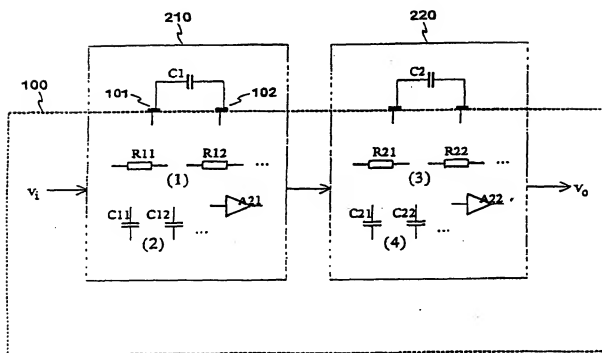


Fig. 2

calibration phases (1), (2), (3) and (4)

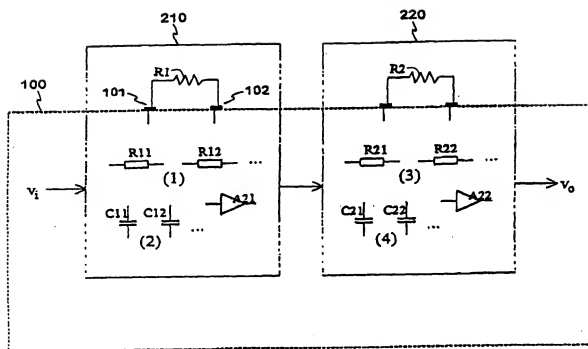


Fig. 2A

calibration phases (1), (2), (3) and (4)

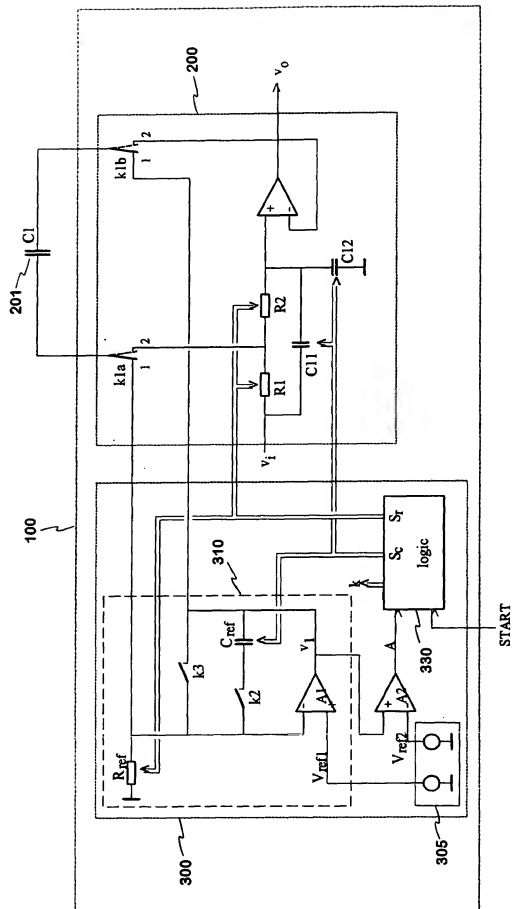


Fig. 3

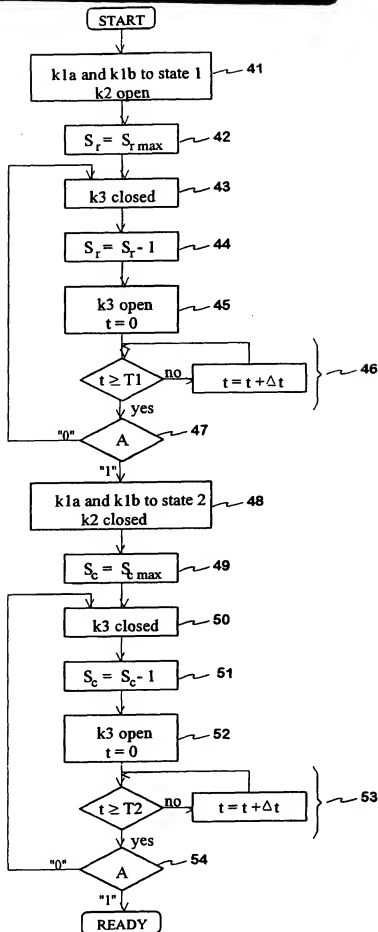


Fig. 4

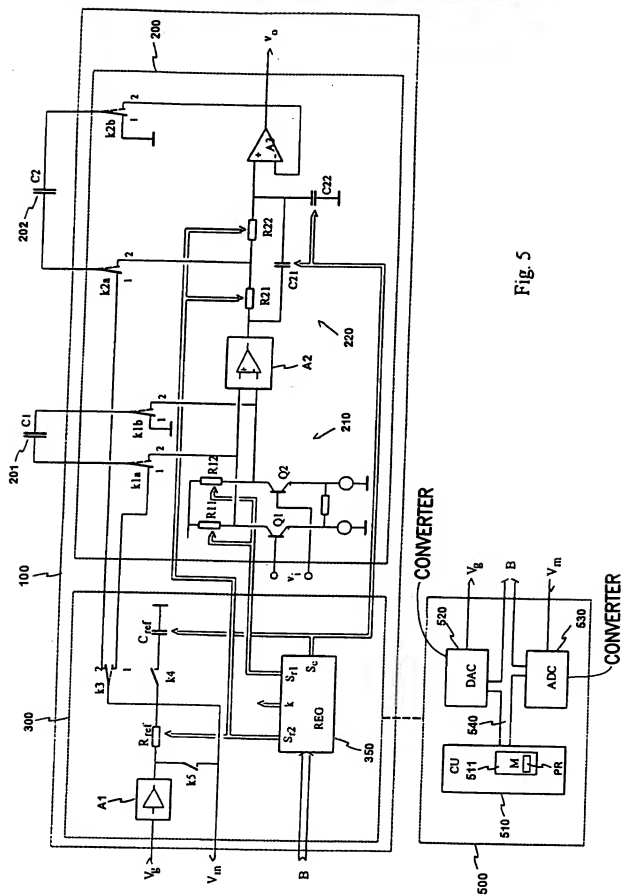


Fig. 5

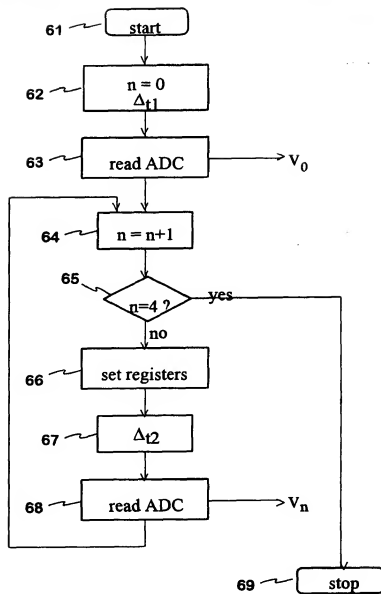


Fig. 6




Fig. 7a

$$S_t = b_0 b_1 b_2 b_3 b_4$$

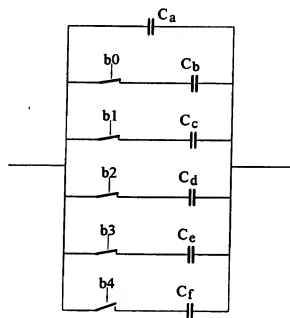


Fig. 7b

$$S_c = b_0 b_1 b_2 b_3 b_4$$